




## KAM® CSM™ CIRCULATING SAMPLE MIXER

**TEL** +1 713 784 0000  
**FAX** +1 713 784 0001  
**Email** Sales@Kam.com

User Guidelines  
CSMMANUAL-0709  
KAM CONTROLS, INC.  
3939 Ann Arbor Drive  
Houston, Texas 77063 USA  
[www.KAM.com](http://www.KAM.com)

# KAM CSM™ CIRCULATING SAMPLE MIXER

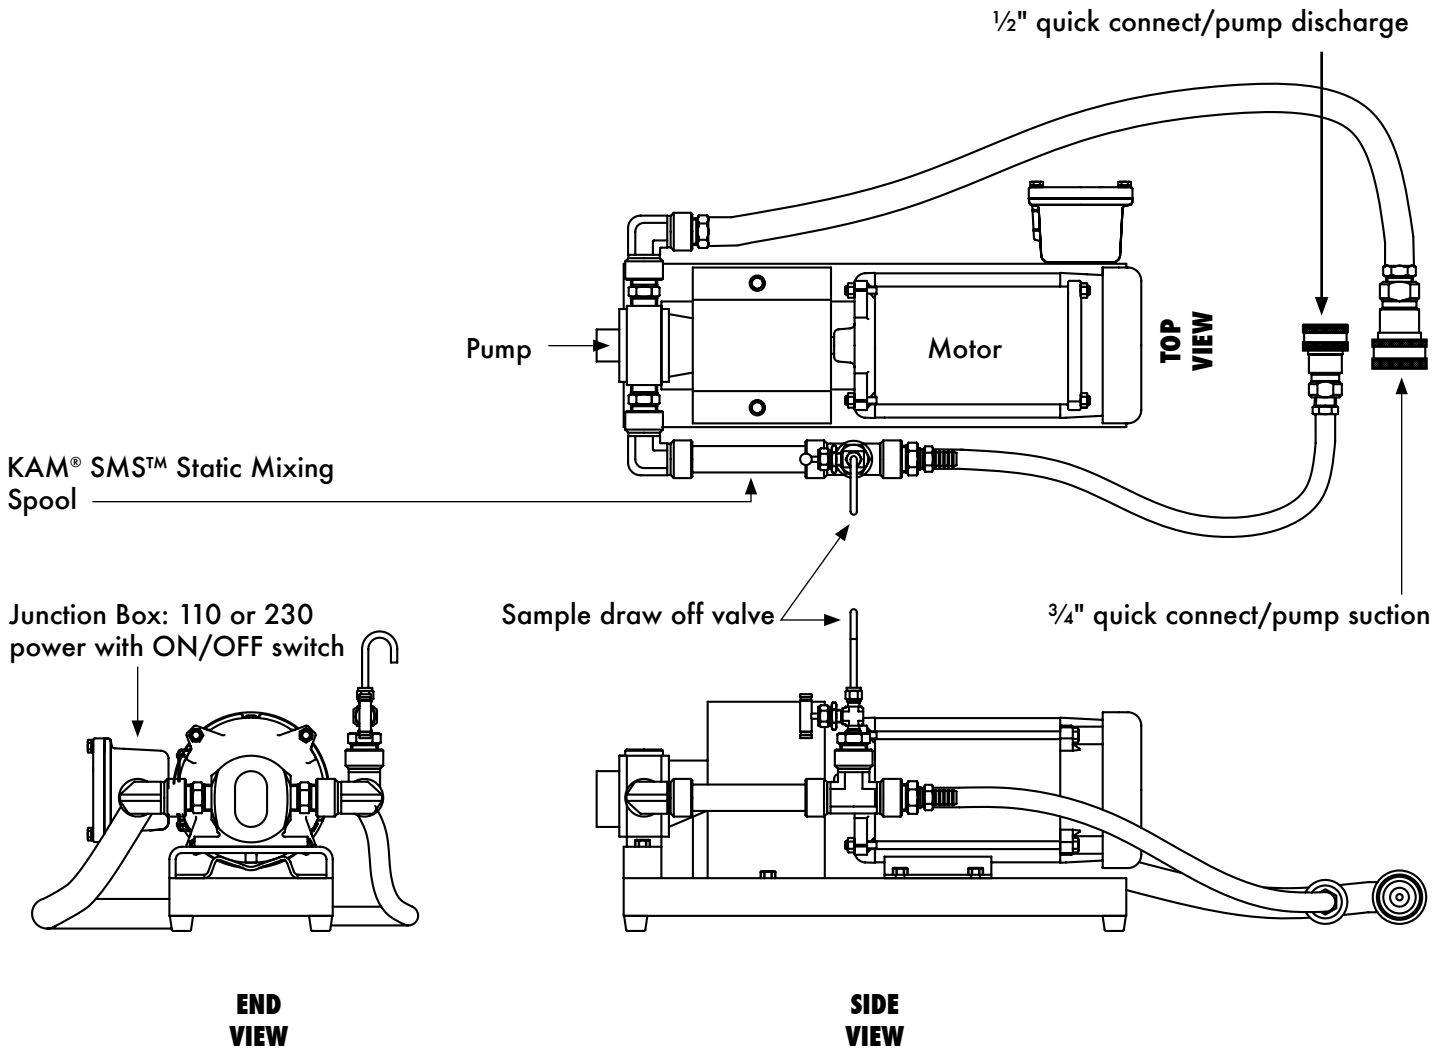

- ▶ Observe all electrical codes
- ▶ Do not run pump dry
- ▶ Do not turn pump on unless both suction and discharge lines are connected to a KAM® SR™ Sample Receiver via quick connects
- ▶ Make sure KAM® SR™ lid is closed and sealed prior to switching on the KAM® CSM™ pump
- ▶ Wear safety glasses at all times when using the sample draw off valve

KAM CONTROLS, INC. reserves the right to make changes to this document without notice.